

PAPER • OPEN ACCESS

Thermography of flame during diesel fuel combustion with steam gasification

To cite this article: I S Anufriev *et al* 2017 *J. Phys.: Conf. Ser.* **925** 012014

View the [article online](#) for updates and enhancements.

Related content

- [Effects of fractal grid on spray characteristics and flame development in burner combustion](#)
S H Amirnordin, A Khalid, M Suardi et al.
- [Interaction of turbulence and chemistry in a low-swirl burner](#)
J B Bell, R K Cheng, M S Day et al.
- [Cellular burning in lean premixed turbulent hydrogen-air flames: Coupling experimental and computational analysis at the laboratory scale](#)
M S Day, J B Bell, R K Cheng et al.

Thermography of flame during diesel fuel combustion with steam gasification

I S Anufriev¹, S S Arsentev^{1,2}, M V Agafontsev³, E P Kopyev¹, E L Loboda³,
E Yu Shadrin¹ and O V Sharypov¹

¹ Institute of Thermophysics. S.S. Kutateladze SB RAS, Novosibirsk, 630090, Russia

² Novosibirsk State University, Novosibirsk, 630090, Russia

³ Tomsk State University, Tomsk, 634050, Russia

E-mail: anufriev@itp.nsc.ru

Abstract. The paper represents a study concerning the combustion of liquid hydrocarbon fuel in a perspective burner device with the controlled forced supply of overheated steam into the combustion zone, using diesel fuel. The thermal imaging measurements are conducted for the outer flame of the burner device in the wide range of regime parameters (flow rate and temperature of steam). A thermal imaging camera (FLIR, JADE J530SB) is used in the experiments. The effective emissivity coefficient of flame is obtained versus the flow rate of steam supplied. The steam parameters are found to influence on the temperature in the outer flame of the burner device.

1. Introduction

Fuel gasification is the conversion of solid or liquid fuel into combustible gases by using the partial oxidation during the high temperature heating [1, 2]. The gasification of organic fuels is used in some cases for processing of low grade fuels to produce a synthesis gas [3]. The synthesis gas obtained is used as a final product for manufacturing purposes, for example as gaseous fuels for thermal electric power stations or as a hydrogen source (for example, the production of ammonia), carbon black, etc. [4-8]. In addition, this gaseous fuel releases a smaller amount of toxic gases during combustion compared to original fuel. Steam is often used as an oxidizer for fuel gasification and the synthesis gas produced is called a water gas.

Also, steam is used as a sprayer in fuel nozzles [9]. This improves the solubilizing of black oil and intensifies its vaporization and combustion. There are the other examples of using steam during the fuel combustion, for example, the supply of steam into the combustion chamber of a gas turbine installation allows the content of toxic nitrogen oxides to be reduced in combustion products due to decreasing the flame temperature [10, 11].

In addition, the injection of water or steam into the combustion chambers of thermal electric power stations (using liquid or solid fuel) is also used to reduce NO_x emissions. There are the examples of the water injection into the internal-combustion engines in automobiles, in order to suppress detonation, decrease carbonization and reduce NO_x and CO concentrations [12, 13]. In all these applications, water (steam) acts as a cooling component used to dilute a fuel mixture, which allows the temperature and the formation of thermal NO_x to be reduced in the combustion zone. However, this method leads



to the decrease in the power and efficiency of equipment, and its use is limited since CO emissions and other products of incomplete fuel combustion start increasing along with the reduction of NO_x . Therefore, the use of steam during the fuel combustion in a certain device requires a comprehensive scientific evidence to select the optimal (according to environmental and thermotechnical specifications) modes and structural parameters.

At the Institute of Thermophysics SB RAS a new method is proposed for fuel combustion with the use of steam, when there is the gasification of carbon-containing particles during the incomplete combustion of liquid hydrocarbons [14]. The supply of overheated steam to the liquid hydrocarbon combustion zone was shown to sharply intensify combustion [15, 16]. This provides stable ignition, high completeness of fuel combustion and a low content of toxic components in combustion products. This method of combustion is promising for utilization of low-grade liquid hydrocarbon fuels and combustible industrial wastes to produce heat energy. In the previous papers [15-17] the authors used an autonomous burner device with constant steam parameters (flow rate and temperature) [18, 19]. However, these characteristics should be adjusted to control the combustion process. In this work a new burner device equipped with an electric steam generator is used to obtain a flow of overheated steam for the wide range of flow rates and temperatures. To study the effect of steam parameters on the main characteristics of the liquid hydrocarbons combustion process (the composition of combustion products and the specific heat release capacity), it is necessary to obtain the data for different combustion modes.

This paper represents the thermal imaging study concerning the flame of a perspective burner device during the combustion of diesel fuel along with the supply of overheated steam to the combustion zone for the wide range of steam parameters.

2. Experimental setup and measurement procedure

The studies were conducted using a combustion stand (figure 1) equipped with a new burner device (10 kW), an electric steam generator (average power of 1.5 kW), a plunger metering pump, an automatic steam generator control system, a fuel supply system, an electronic balance to control the flow of water and fuel, as well as with necessary control and measurement instruments.

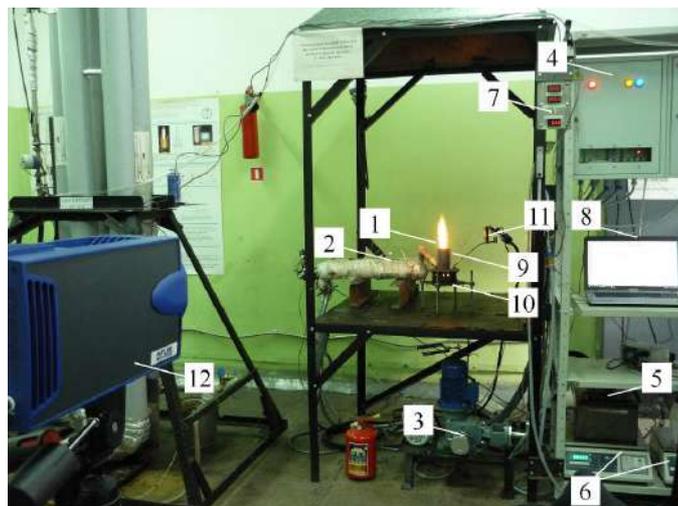


Figure 1. Combustion stand for the study of liquid hydrocarbon combustion with steam gasification: 1 is the burner device, 2 is the electric steam generator, 3 is the plunger metering pump, 4 is the automatic steam generator control system, 5 is the fuel supply system, 6 is the electronic balance, 7 is the indicators of control and measurement instruments, 8 is the computer, 9 is the gas-generation chamber of the furnace unit, 10 is the combustion chamber of the furnace unit, 11 is the fuel pipe, 12 is the thermal imager

The main elements of the new burner device are: a cylindrical body, a combustion chamber, a steam nozzle and a gas-generation chamber. The combustion chamber has holes for the air inflow from the atmosphere. Fuel is supplied into the combustion chamber through the fuel pipe. The stable rate of fuel is provided by the fuel nozzle and the pump and controlled by the electronic balance. A steam nozzle is mounted coaxially above the combustion chamber near the base of the gas-generation chamber and is oriented vertically (outlet diameter is 0.5 mm). The steam nozzle is connected with an external steam generator. The test burner is a vaporizing burner according to the operation principle. The combustion process is similar to the operation of an autonomous burner [17].

The steam generator consists of three heating units connected in sequence. Each unit is a metal tube (38 mm in external diameter) with a length of 0.5 m and a wall thickness of 8 mm. An electric tubular U-shaped heater (maximum power of 700 W) was mounted inside the pipe. The space between the heater and the pipe wall was filled with periclase DM-1 to increase heat transfer. In the wall of each pipe there are the closed rectangular cross-section channels (4×2 mm and 6 m in length for each block) in the form of spiral. The pipes are insulated outside. The monitoring temperature sensors are installed on the surface of each block. The mass flow of water (steam) is provided by the plunger metering pump and controlled by the electronic balance. The steam temperature is regulated by changing the power of the heaters. The pressure in the steam generator is recorded by the digital pressure sensor. The developed laboratory electric steam generator produces the overheated steam in the range of the temperature and flow rate of 100÷600 °C and 0.25÷1.5 kg/h (pressure up to 10 atm).

The thermal imaging camera (FLIR, JADE J530SB) was used to measure the temperature in the high temperature flame of the burner device. This device has a high temporal resolution: the frame rate up to 177 Hz with a maximum resolution of 320×240 pixels and up to 18 kHz with a resolution of 320×4 pixels. The minimum time of frame exposure is 6 μs. The operating range of the thermal imager is in the middle infrared range of 2.5-5.0 microns. The same spectral range contains the powerful flame radiation lines caused by the radiation of hot combustion products (including water vapors, CO₂, and CO). Based on the results of previous studies [20], a narrow spectral band dispersion optical filter F0616 with bandwidth of 2.5-2.7 microns was selected for operation.

The filter was selected due to the powerful emission lines of water vapors and CO₂ in this spectral range. The temperature measurement range of the thermal imager is determined by calibration and reaches 583-1773 K for the filter selected. The data collection and initial processing of thermograms were carried out using a specialized program, Altair. The factory calibrations were used for the F0616 filter with an exposure time of 9, 64, and 350 μs for the operation of the thermal imager. The previous spectral analysis of the flame temperature and pressure [20] demonstrated the absence of peak periodic oscillations in the test flame. To obtain an average temperature value, the measurements were conducted with a frequency of 50 Hz for 1 min.

To determine the effective emissivity coefficient simultaneously with the thermal imager measurements at the control points (on the axis of the burner device $r = 0$, at the height $x = 30$ mm from the edge of the burner), the temperature was recorded using a platinum-platinum rhodium type B thermocouple (600...1600 °C) with the thermoelectrodes 300 microns in diameter. The thermal inertia of the thermal converter was not more than 5 seconds. The permitted deviation limits of thermoelectromotive forces were ± 0.005 compared with the standard static characteristics of the converter for the value of the measured temperature. Using the thermogram, the average temperature was determined in the area of hot junction. The effective emissivity coefficient, the values of which were ranged from 0.3 to 0.65 depending on the steam flow, was selected using the Altair software. The value of the effective emissivity coefficient obtained was used for the entire area.

3. Measurement results and analysis

Measurements were carried out under different operating conditions of the burner device. For the constant rate of fuel $F_f = 0.82$ kg/h, the value $\gamma = F_v / (F_v + F_f)$ was varied in the range of 0.24÷0.56, where F_v is the average mass flow rate of steam. The steam temperature was varied in the range of $T_v = 160\div 560$ °C for each value of F_v .

Figure 2 shows the time-average temperature profiles in the outer flame of the burner device for different flow rates of steam at $T_v = \text{const}$. It should be noted that the flame is a translucent three-dimensional optical medium, so the thermal imager detects the integral radiation of all inner medium layers. This integral radiation is required to determine the temperature in the observation plane, using the calibrations and the effective emissivity coefficient. The thermograms shown in figure 2 demonstrate a significant effect of the supplied steam flow both on the temperature distribution in the outer flame and the flame dimensions (photographs in figure 2).

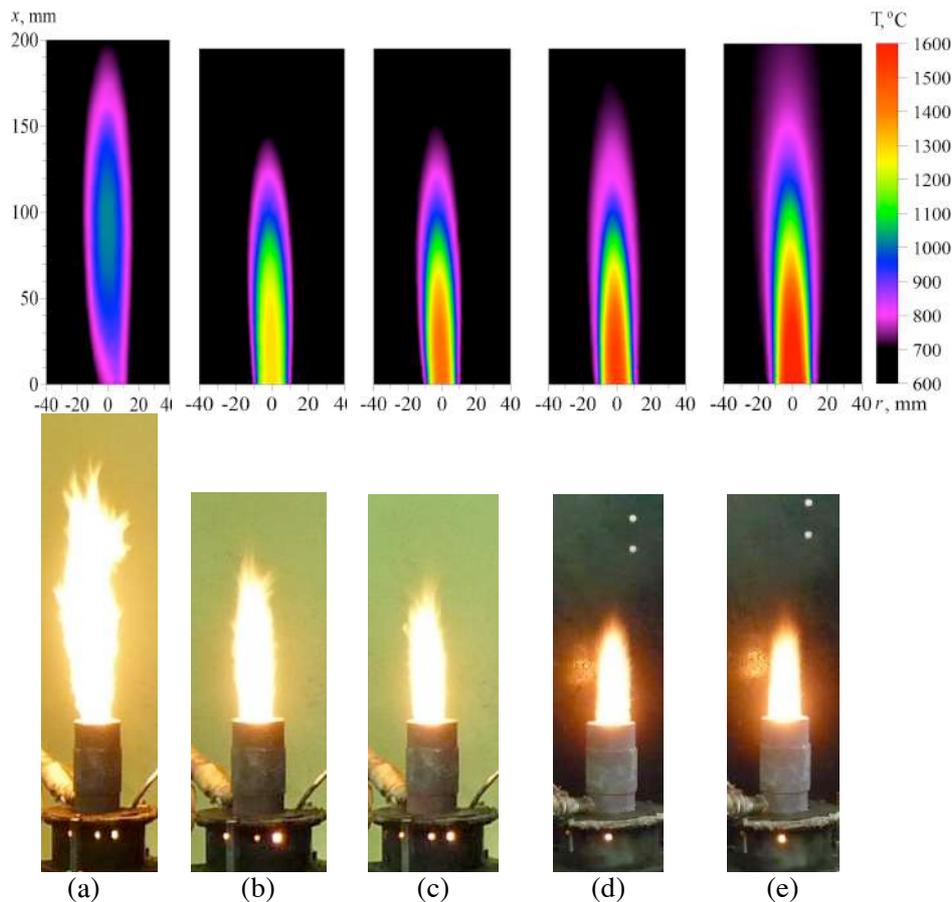


Figure 2. Thermograms of flame and the photographs for different steam flow rates (at a constant temperature steam $T_v \sim 250$ °C: $\gamma = 0.24$ (a), $\gamma = 0.34$ (b), $\gamma = 0.44$ (c), $\gamma = 0.50$ (d), $\gamma = 0.56$ (e), and a steam pressure in the range of 8 ± 2 atm, respectively)

Figure 3 shows the flame temperature versus the height at the different flow rates and temperatures of steam supplied ($\gamma = 0.56$). The analysis of the results shows (Figure 3a), that the maximum flame temperature (T_{max}) is achieved at a maximum flow rate of steam ($\gamma = 0.56$). At the same time, a longitudinal size of the luminous area is minimal (photograph in figure 2d). (The experiments showed that a further increase in the γ parameter led to the blowout of flame, and a low flow rate of steam ($\gamma < 0.3$) led to the incomplete combustion of fuel). The maximum flame temperature increases with the increase in the steam temperature (figure 3b).

For the modes with a high value of the parameter γ the height dependence of the flame temperature is monotonous, and the maximum is reached at the outlet of the burner. When $\gamma \leq 0.5$ the maximum temperature is observed at some distance from the outlet of the burner, which indicates the incomplete mixture combustion before the release into the atmosphere.

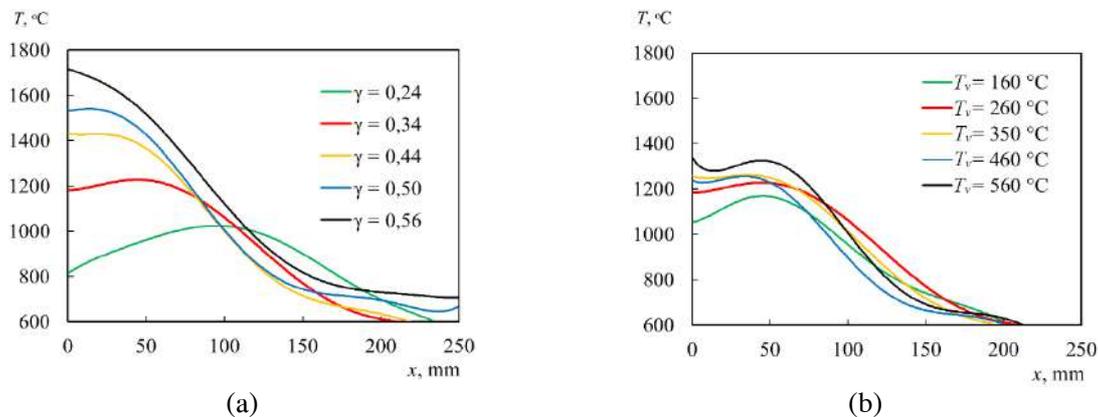


Figure 3. Distribution of the time-average temperature in the outer flame along the vertical center line of the flame for different mode parameters: (a) the steam flow rate is varied, $T_v = 250 ^\circ\text{C}$; (b) the steam temperature is varied, $\gamma = 0.34$, the steam pressure is 4 atm

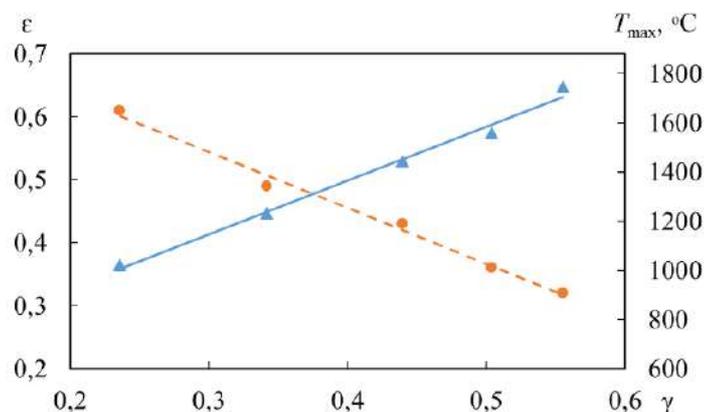


Figure 4. Effective emissivity coefficient of flame (\bullet) and maximum temperature (\blacktriangle) in the outer flame versus the γ parameter, $T_v = 250 ^\circ\text{C}$

The emissivity coefficient of flame ϵ was determined versus the flow rate of the steam supplied (figure 4): the value ϵ decreases with increasing the γ parameter. The γ parameter dependence of the maximum flame temperature is also linear, but increases with increasing γ (figure 4).

4. Conclusion

With the use of thermography, thermal characteristics in the flame of the prospective burner device were studied when diesel fuel was burned with forced regulated feeding of superheated steam to the combustion zone. Thermal imaging measurements were carried out over a wide range of the operating parameters (flow rate and temperature of the supplied water vapor). It has been established that the consumption of superheated water vapor has a significant influence both on the temperature distribution in the flame and on its dimensions. The maximum temperature was reached at the maximum steam flow rate and was $1700 ^\circ\text{C}$. The dependence of the temperature of the flame on the temperature of the vapor turned out to be weaker. The dependence of the effective coefficient of flame emission on the flow rate of the supplied steam was also established.

The experimental data obtained can be used for the measurement analysis of the gas composition in combustion products and the heat release, in order to provide a scientific evidence for the selection of the energy-efficient and environmentally friendly utilization ways for off-grade liquid hydrocarbons to produce thermal energy.

References

- [1] Higman C and Van Der Burgt M 2008 *Gasification*. (2nd ed.) (Gulf Professional Publishing)
- [2] Lavrov N V and Shurygin A P 1962 *Introduction to the theory of fuel combustion and gasification* (Acad. Sciences of the USSR, Moscow)
- [3] Rostrup-Nielsen J and Christiansen L J 2011 *Concepts in Syngas Manufacture* (Imperial College Press, London)
- [4] Liu K, Song Ch and Subramani V 2010 *Hydrogen and Syngas Production and Purification Technologies* (John Wiley & Sons, Inc., Hoboken, New Jersey)
- [5] Rezaian J and Cheremisinoff N 2005 *Gasification Technologies: A Primer for Engineers and Scientists* (Taylor & Francis)
- [6] Emanuele Graciosa Pereira, Jadir Nogueira da Silva, Jofran L. de Oliveira, Cssio S. Machado 2012 *Renewable and Sustainable Energy Reviews* **16** 4753
- [7] Ryabtsev I I and Volkov A E 1968 *Gas production from liquid fuels for synthesis of ammonia and alcohols* (Khimiya, Moscow)
- [8] Andreev F A, Kargin S I, Kozlov L I and Pristavko V F 1974 *Combined nitrogen technology* (Khimiya, Moscow)
- [9] Khzmlyan D M and Kagan J A 1976 *Combustion theory and furnace arrangements* (Energia, Moscow)
- [10] Tsanev S V, Burov V D and Remezov A N 2002 *Gas turbine and steam-gas plants of thermal power stations* (MEI, Moscow)
- [11] Ivanov A A, Ermakov A N and Shlyakhov R A 2010 *Izv. RAN. Energetika* **3** 119
- [12] Lerner M O 1981 *Khimiya i zhizn'* **5** 16
- [13] Efremov P K 1977 *Proc. of the All-Union Scientific Conference «Protection of air pool from pollution by toxic emissions vehicles»* **1** 93
- [14] Vigriyanov M S, Salomatov V V and Alekseenko S V 2003 *RF Patent* **2219435M.S.**
- [15] Alekseenko S V, Pashchenko S E and Salomatov V V 2010 *J. Engng. Physics and Thermophysics* **83** 729
- [16] Alekseenko S V, Anufriev I S, Vigriyanov M S, Dulin V M, Kopyev E P and Sharypov O V 2014 *Thermophys. Aeromech* **21** 393
- [17] Alekseenko S V, Anufriev I S, Vigriyanov M S, Kopyev E P and Sharypov O V 2016 *Combust. Expl. Shock Waves* **52** 286
- [18] Vigriyanov M S, Alekseenko S V, Anufriev I S and Sharypov O V 2014 *RF Patent* **2523591**
- [19] Vigriyanov M S, Alekseenko S V, Anufriev I S and Sharypov O V 2016 *RF Patent* **2579298**
- [20] Anufriev I S, Kopyev E P and Loboda E L 2014 *Proc. SPIE 9292 «20th International Symposium on Atmospheric and Ocean Optics: Atmospheric Physics»* **929226**